


# SAMPLING LINE FOR ORGANIC GAS IN EMISSION

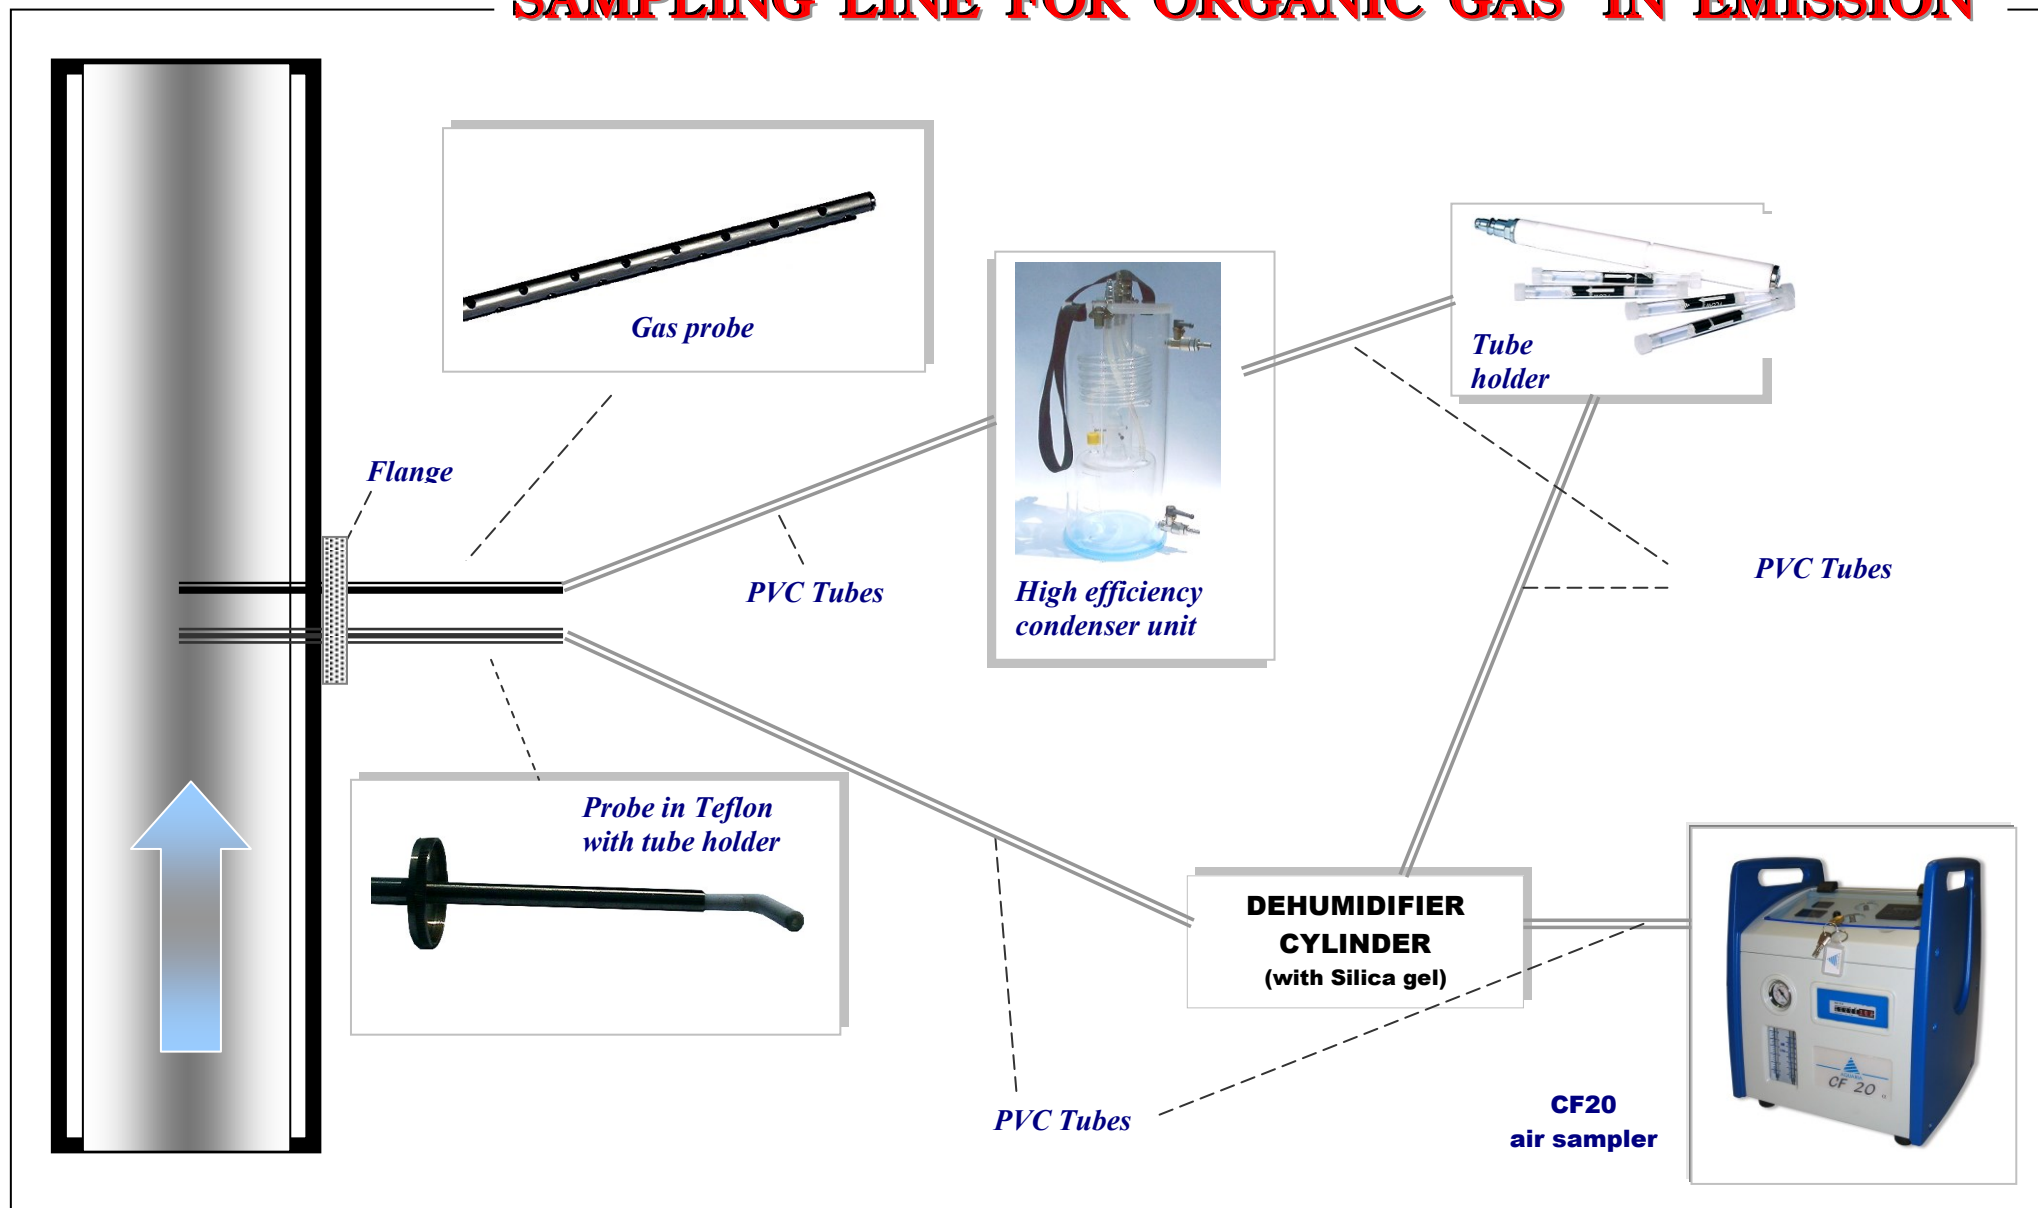

**NOTE:** *The Teflon probe can be used only to maximum temperatures of 150 ° C  
The Teflon probe and the tube holder must be completed with a activated carbon or silica gel tube  
The condenser is indicated for the condensate sampling for a subsequent analysis (recommended in case of flue gas with a high water vapour content)*